


# Instrument hoses, accessories, and replacement parts

Device type

supply hose

Instrument

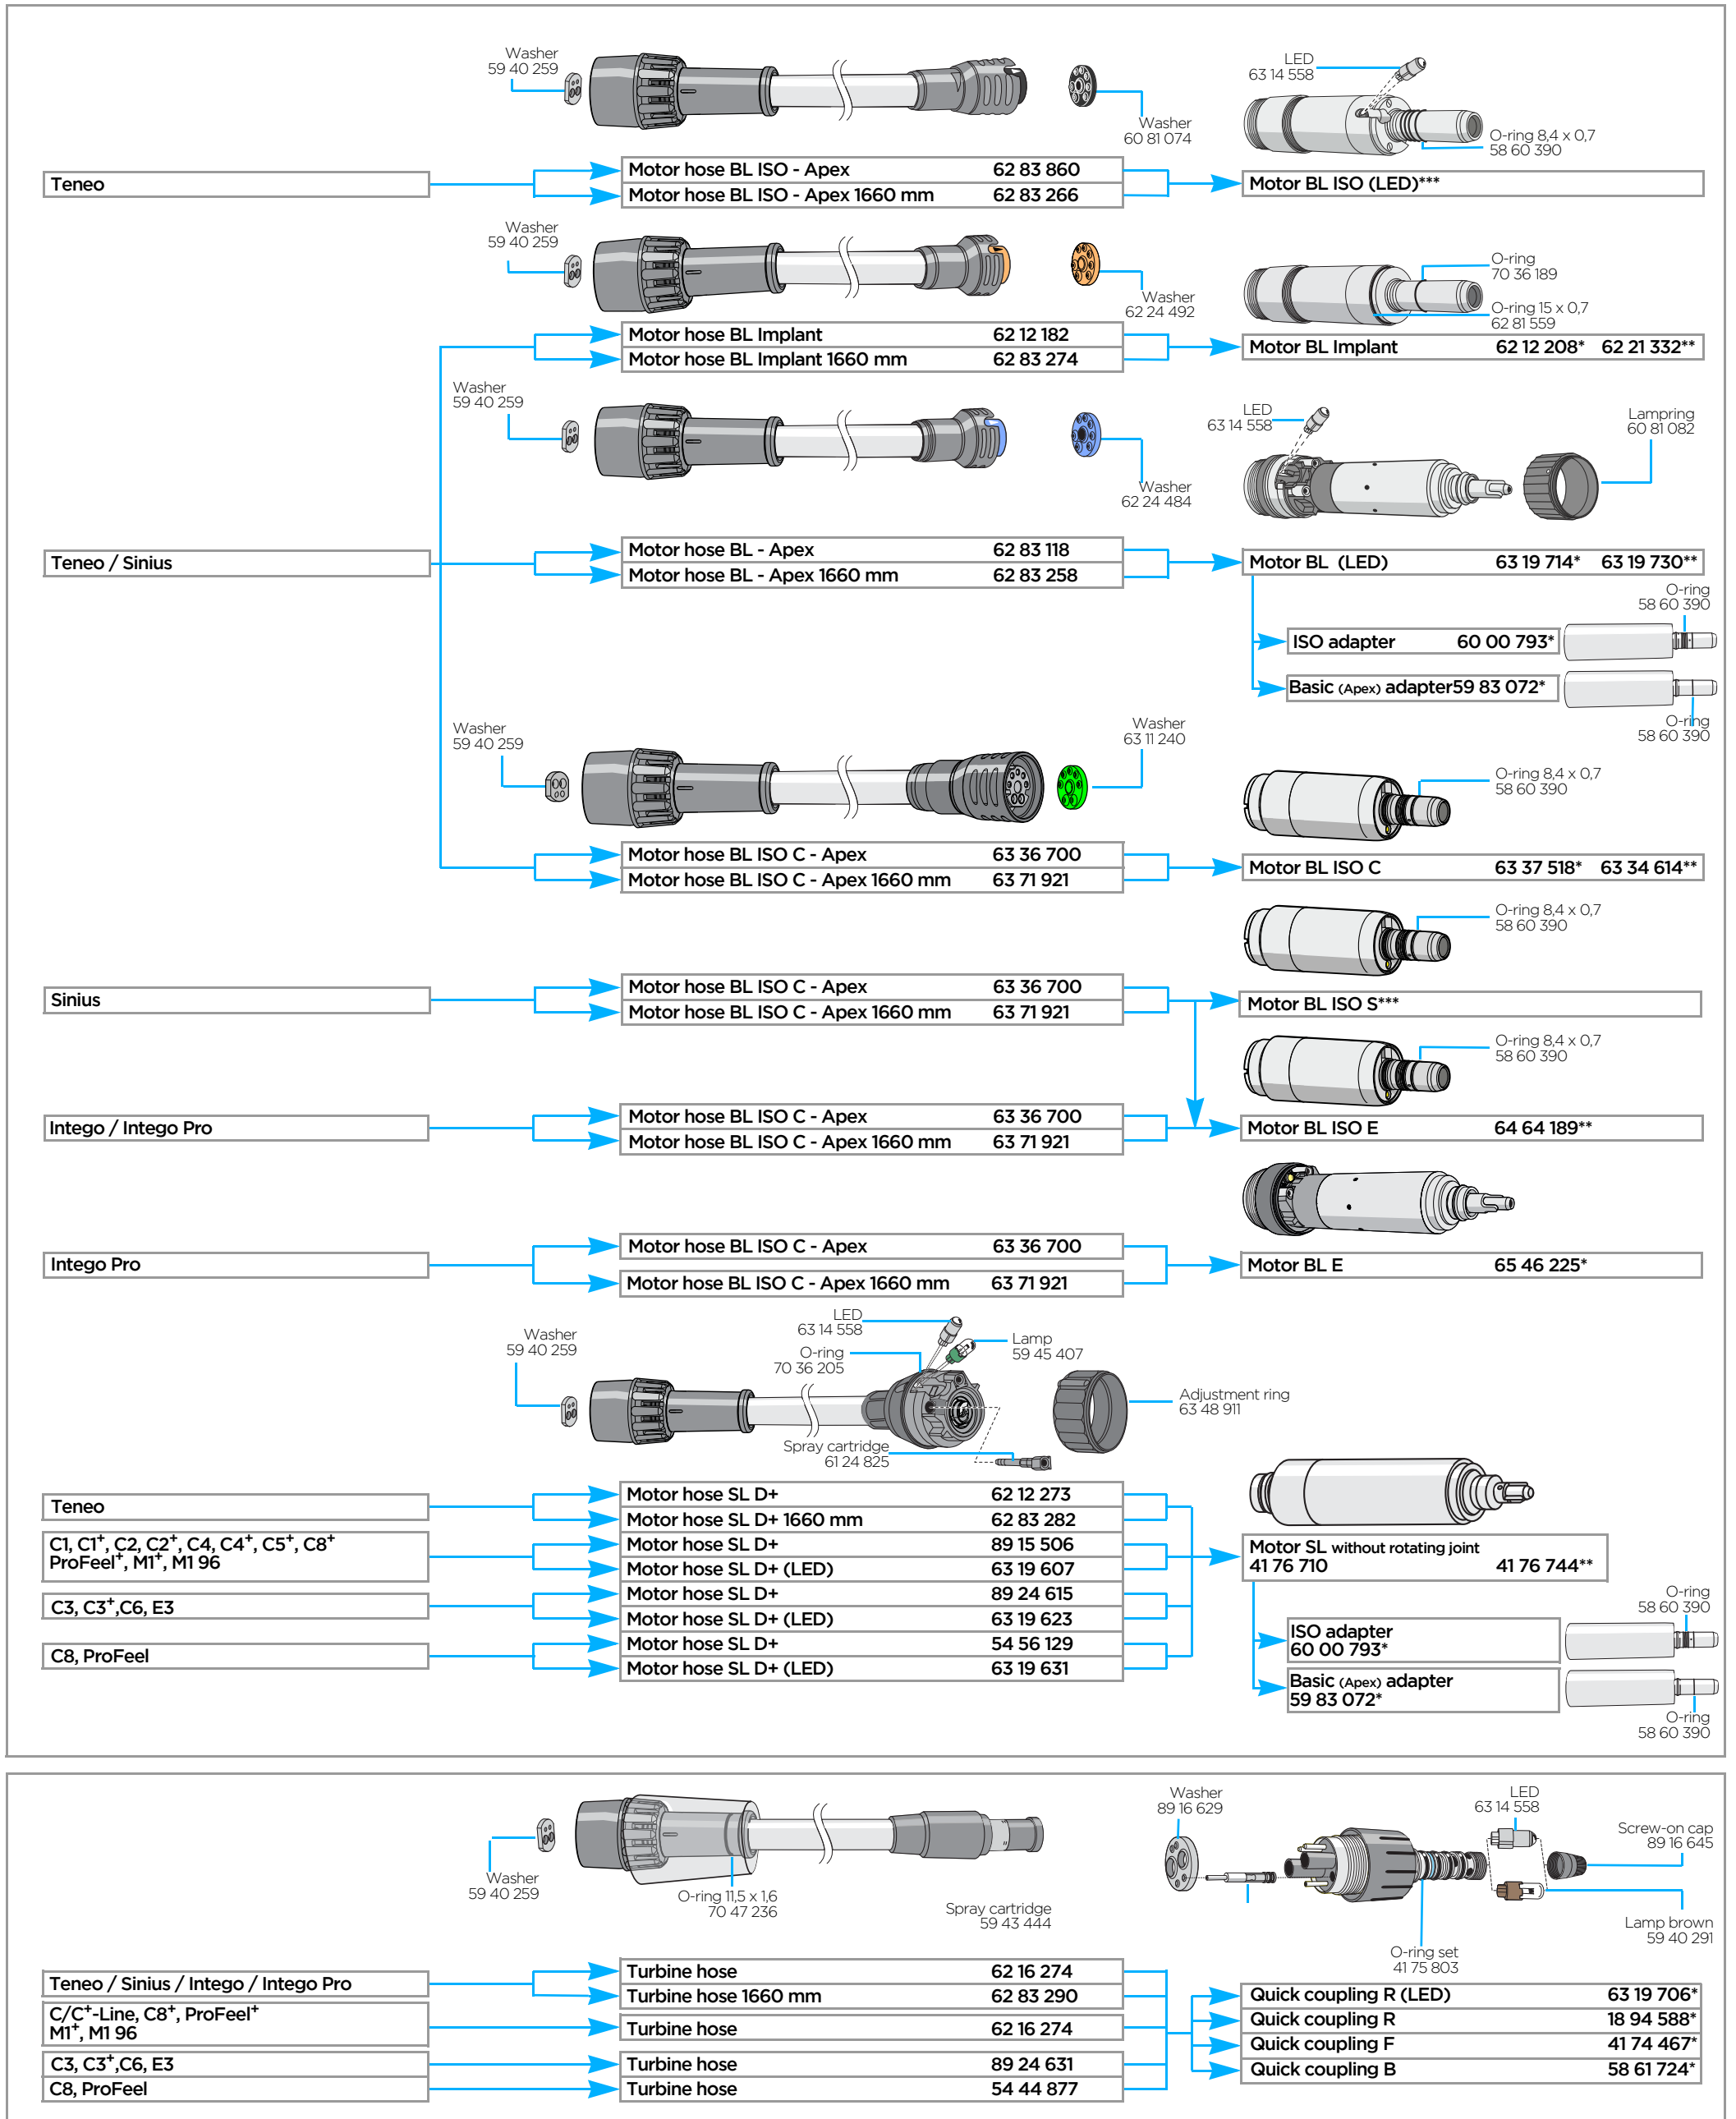

\* Individual repairs possible, address for individual repairs: Instrumenten-Service-Center ISC, Fabrikstraße 35, D-64625 Bensheim  
 \*\* Repair/Exchange: Low cost and fast processing  
 \*\*\* discontinued

You will find the Sirona repair order here:  
<https://www1.dentsplysirona.com/en/products/instruments/instrument-service-center.html>

# Instrument hoses, accessories, and replacement parts

Device type

supply hose

Instrument

Teneo / Sinius	<ul style="list-style-type: none"> <li>SiroSonic TL hose (LED) 62 12 174</li> <li>SiroSonic TL hose 1660 mm (LED) 62 83 316</li> </ul>	<ul style="list-style-type: none"> <li>SiroSonic TL Handpiece 62 12 216</li> </ul>
Intego / Intego Pro	<ul style="list-style-type: none"> <li>SiroSonic L hose E (LED) 64 45 998</li> </ul>	<ul style="list-style-type: none"> <li>SiroSonic L Handpiece (dark blue) 59 13 509</li> </ul>

C1, C1+, C2, C2+, C4, C4+, C5+, C8+, ProFeel+, M1+, M1 96	<ul style="list-style-type: none"> <li>SiroSonic L (bu) 59 21 031</li> <li>SiroSonic L (LED) 63 19 664</li> </ul>	<ul style="list-style-type: none"> <li>SiroSonic L Handpiece (dark blue) 59 13 509</li> <li>SiroSonic (without light) 59 13 517</li> </ul>
C3, C3+, C6	<ul style="list-style-type: none"> <li>SiroSonic L (bu) 59 21 056</li> <li>SiroSonic L (LED) 63 19 672</li> </ul>	
C8	<ul style="list-style-type: none"> <li>SiroSonic (bu) 59 21 080</li> </ul>	
ProFeel	<ul style="list-style-type: none"> <li>SiroSonic L (bu) 59 21 122</li> </ul>	

Sinius / Teneo starting with Serial No. 120.000 (or with NAJ control 6535590)	<ul style="list-style-type: none"> <li>Sprayvit M hose 63 21 686</li> <li>Sprayvit M hose 1660 mm 63 29 846</li> </ul>	<ul style="list-style-type: none"> <li>Sprayvit M valve body 63 21 983</li> <li>↳ 1x Heating cartridge + O-ring + Lamp + LED</li> </ul>
Intego / Intego Pro	<ul style="list-style-type: none"> <li>Sprayvit E hose 64 45 972</li> </ul>	<ul style="list-style-type: none"> <li>Sprayvit E valve body 64 53 679</li> <li>↳ LED</li> </ul>
Teneo up to Serial No. 120.000	<ul style="list-style-type: none"> <li>Sprayvit L hose 62 16 282</li> <li>Sprayvit L hose 1660 mm 62 83 308</li> </ul>	<ul style="list-style-type: none"> <li>Sprayvit valve body 41 76 629</li> <li>↳ 2x Heating cartridge + O-ring</li> </ul>
C1, C1+, C2, C2+, C4, C4+, C5+, M1+, C3, C3+, C6	<ul style="list-style-type: none"> <li>Sprayvit L hose 62 16 282</li> <li>Sprayvit L hose 41 77 759</li> </ul>	
C8+, ProFeel+	<ul style="list-style-type: none"> <li>Sprayvit L AE 59 51 582</li> <li>Sprayvit L HE 54 56 053</li> </ul>	<ul style="list-style-type: none"> <li>Sprayvit C8 valve body 60 02 203</li> <li>↳ 2x Heating cartridge + O-ring + Lamp</li> </ul>
C8, ProFeel	<ul style="list-style-type: none"> <li>Sprayvit AE 54 56 004</li> <li>Sprayvit HE 54 56 053</li> </ul>	

Nozzle G with light 59 92 180	Nozzle short with light 41 77 783
Nozzle G without light 59 92 206	Nozzle short without light 59 92 198

\* Individual repairs possible, address for individual repairs: Instrumenten-Service-Center ISC, Fabrikstraße 35, D-64625 Bensheim  
 \*\* Repair/Exchange: Low cost and fast processing  
 \*\*\* discontinued

You will find the Sirona repair order here:  
<https://www1.dentsplysirona.com/en/products/instruments/instrument-service-center.html>